

## NPPTL COVID-19 Response: International Respirator Assessment

Manufacturer: Wenzhou Younuo Protective Product Co., Ltd.

Model Tested: Foldable Ear Loop KN95

Date Tested: September 30, 2020

These findings pertain to the Wenzhou Younuo Protective Product Co., Ltd., model Foldable Ear Loop KN95. The packaging for this product indicates that it meets GB2626-2006 (the Chinese standard for Respiratory Protective Equipment – Non-Powered Air-Purifying Particle Respirator).

Ten respirators were submitted for evaluation. The samples were tested using a modified version of NIOSH Standard Test Procedure (STP) TEB-APR-STP-0059. This modified assessment plan can be found [here](#).

No certificate of approval was provided with the samples received; therefore, the authenticity of the claims cannot be validated.

The maximum and minimum filter efficiency was 97.20% and 33.30%, respectively. One respirator measured more than 95%. Nine respirators measured less than 95%.

While the above-listed product classification has similar performance requirements to NIOSH-approved devices, NIOSH does not have knowledge about the sustained manufacturer quality system and product quality control for these products. NIOSH also does not have knowledge about the product's handling and exposures after leaving its manufacturer's control.

In addition, this product is an ear loop design. Currently, there are no NIOSH-approved products with ear loops; NIOSH-approved N95s have head bands. Furthermore, limited assessment of ear loop designs, indicate difficulty achieving a proper fit. While filter efficiency shows how well the filter media performs, users must ensure a proper fit is achieved.

**This assessment is not a part of the NIOSH respirator approval process and will in no way lead to or preclude NIOSH approval through the official approval process.** This assessment was developed as an assessment of the filter efficiency for those respirators represented as certified by an international certification authority, other than NIOSH, to support the availability of respiratory protection to US healthcare workers due to the respirator shortage associated with COVID-19. Only particulate filter efficiency was assessed.

The results provided in this letter are specific to the subset of samples that were provided to NPPTL for evaluation.

These results will be used to update the CDC guidance for [Crisis Capacity Strategies \(during known shortages\)](#).

## Evaluation of International Respirators

**Test:** Modified TEB-APR-STP-0059

**Date Tested:** September 30, 2020

**Report Prepared:** September 30, 2020

**Manufacturer:** Wenzhou Younuo Protective Product Co., Ltd.

**Item Tested:** Foldable Ear Loop KN95

**Country of Certification:** China (GB2626-2006)

Pictures have been added to the end of this report.

Filter	Flow Rate (LPM)	Initial Filter Resistance (mmH <sub>2</sub> O)	Initial Percent Leakage (%)	Maximum Percent Leakage (%)	Filter Efficiency (%)
1	85	7.9	52.7	52.8	47.20
2	85	9.7	2.09	2.80	97.20
3	85	13.9	8.95	14.8	85.20
4	85	9.9	9.17	9.17	90.83
5	85	7.9	50.1	50.5	49.50
6	85	13.4	7.92	7.92	92.08
7	85	10.5	8.33	8.33	91.67
8	85	10.3	8.85	8.85	91.15
9	85	6.0	66.3	66.7	33.30
10	85	11.7	8.28	8.28	91.72
<b>Minimum Filter Efficiency: 33.30%</b>			<b>Maximum Filter Efficiency: 97.20%</b>		


- The test method utilized in this assessment is not the NIOSH standard test procedure that is used for certification of respirators. Respirators assessed to this modified test plan do not meet the requirements of STP-0059, and therefore cannot be considered equivalent to N95 respirators that were tested to STP-0059.
- Respirators tested may not be representative of all respirators with the same certification mark. NIOSH has no control over suppliers and distributors of respirators certified by other national or international parties.
- This assessment is not a confirmation that it conforms with any or all of its specifications in accordance with its certification mark.
- This assessment was not a part of the NIOSH approval program. These results do not imply nor preclude a future approval through the NIOSH respirator approval program.

NPPTL COVID-19 Response: International Respirator Assessment



**BFE≥95% ★★★★★**  
**KN95**  
**PROTECTIVE MASK**

Personal protective equipment  
intended for general or industrial use.




Store in dry, well-ventilated, sanitary area  
Safe storage conditions:  
-5°C/23°F to 50°C/122°F  
Maximum relative humidity 85%

Ingredient: none-woven fabric, filter carton, polypropylene, melt-blown filter fabric.  
Model No.: Foldable ear-loop KN95  
Spec.: 15x11.3cm  
Executive Standard: GB2626-2006  
Production Date/Lot: Please see certificate of inspection inside the box  
Shelf Life: 2 years  
Non-medical use

DIST BY: **USA:** Bellapierre Cosmetics Inc.  
20417 Nordhoff St., Chatsworth CA 91311  
**United Kingdom:** Bellapierre cosmetics Ltd.  
Unit 8, Meridian Business Park, Fleming Road,  
Waltham Abbey EN9 3BZ  
[www.bellapierre.com](http://www.bellapierre.com)

Manufactured by: Wenzhou Younuo Protective Product Co., Ltd.  
Below miaotou Village, Kunyang Town, Pingyang county,  
Wenzhou, Zhejiang, 325400  
Made in China


**BFE≥95% ★★★★★**  
**KN95**  
**INSTRUCTIONS:**

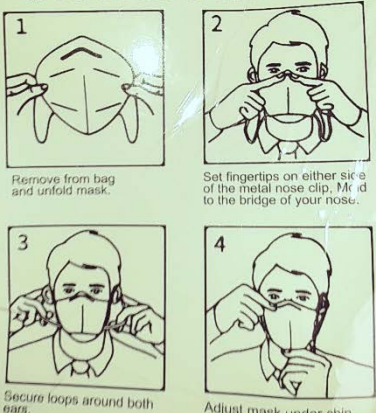

1 Remove from bag and unfold mask.  
2 Set fingertips on either side of the metal nose clip. Press to the bridge of your nose.  
3 Secure loops around both ears.  
4 Adjust mask under chin.

Personal protective equipment  
intended for general or industrial use.

Warning: People with medical conditions such as respiratory or cardiac illnesses should consult with their doctor before use. This product cannot be used as a gas mask in a toxic environment.



# NPPTL COVID-19 Response: International Respirator Assessment



NPPTL COVID-19 Response: International Respirator Assessment



NPPTL COVID-19 Response: International Respirator Assessment



NPPTL COVID-19 Response: International Respirator Assessment

